


Multi Pitting Corrosion

I- Introduction

The effect of the corrosion in our daily life can be underlined by its cost for the society. For an industrial country, the cost is estimated at 3-4% of gross domestic product.

Most metals are sensitive to corrosion in the presence of oxygen and humidity. The general equation of this oxidative process is described as follows:



Corrosion is a general term which generalizes various kinds of processes, such as:

- uniform corrosion: corrosive attack on the entire surface area,
- crevice corrosion: localized corrosive attack caused by oxygen,
- galvanic corrosion: corrosion caused by two different materials in contact,
- pitting corrosion: localized corrosive attack caused by aggressive anion.

In this note, only the pitting corrosion in presence of chloride is investigated. For this purpose, Linear Polarization (LP) and Multielectrode Potentiodynamic Pitting (MPP) are performed.

II- Experimental conditions

Investigations are carried out with a VMP3 and EC-Lab[®] software with 3% NaCl at room temperature in aerated water. Before measurements, the electrodes were polished for 5 minutes using the PK-3 Electrode Polishing kit and rinsed by distilled water and alcohol.

A multi-working electrode set-up is required. In order to overcome the connection complexity due to the multielectrode investigation, N'Stat Box is used (Fig. 1). Note that the utilization of such a device requires the "CE to ground" connection (Fig. 2) which is described in technical note #23 [1]. Electrodes are as follows:

- 4 working electrodes made of steel,
- Ag/AgCl electrode as a reference electrode,
- platinum wire as a counter electrode.



Fig. 1: N'Stat Box.




Fig. 2: "CE to ground connection" in "Advanced Settings" window.

Note: All settings and raw data files presented hereafter are available in the Data Sample folder of EC-Lab[®] Software as LP_03.mpr, LP_04.mpr, LP_05.mpr, LP_12.mpr, MPP_03.mpr, MPP_04.mpr, MPP_05.mpr, and MPP_12.mpr,

III- Results

III-1 LP investigations

LP investigations are performed in the anodic area using slow scan rate (Fig. 3) in order to be under steady-state condition [2]. Moreover, it is important to note that the E range is reduced from -2 V to 2 V in order to optimize the potential resolution to 100 μV . Measured current is averaged in order to reduce noise.

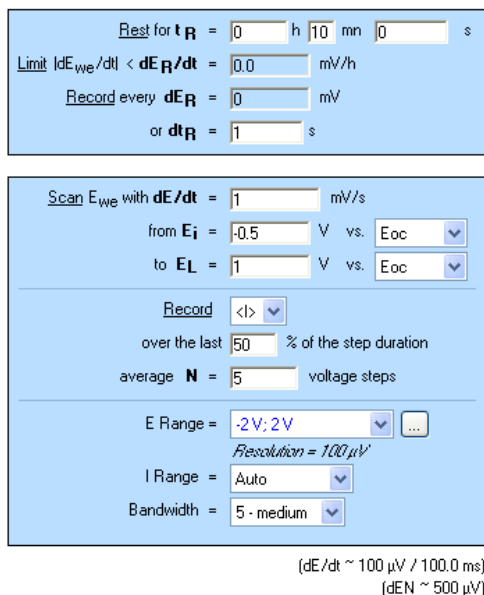


Fig. 3: “Parameters Settings” window for LP measurement.

From LP curves (Fig. 4), it is possible to determine the corrosion potential (E_{corr}) and other related parameters, such as corrosion current (I_{corr}), cathodic (β_{c}) and anodic (β_{a}) Tafel constant and corrosion rate with the “Tafel Fit” analysis tool. Moreover, the pitting potential (E_{p}) can be directly determined by tracking the cursor on the graph and by right clicking on the pitting potential (Fig. 5).

Analysis of Table 1 shows similar E_{corr} for the four electrodes included between -1,152 and -1,000 mV vs. Ag/AgCl with -1,078 mV as mean. Concerning E_{p} , values are included between -760 and -740 mV vs. Ag/AgCl with an average of -747 mV vs. Ag/AgCl.

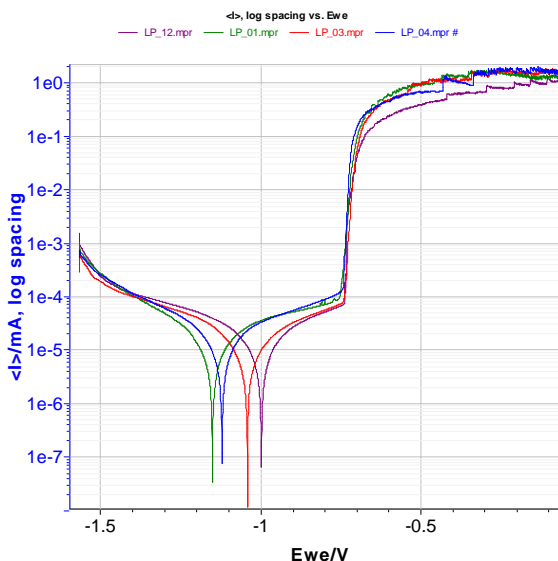


Fig. 4: Four-electrode LP curves.

An example of data determination is shown in Fig. 5. All results are summarized in Table 1.

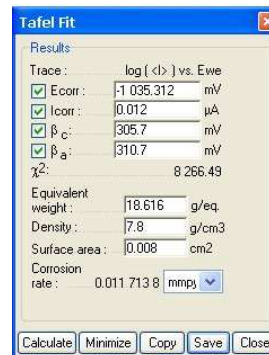
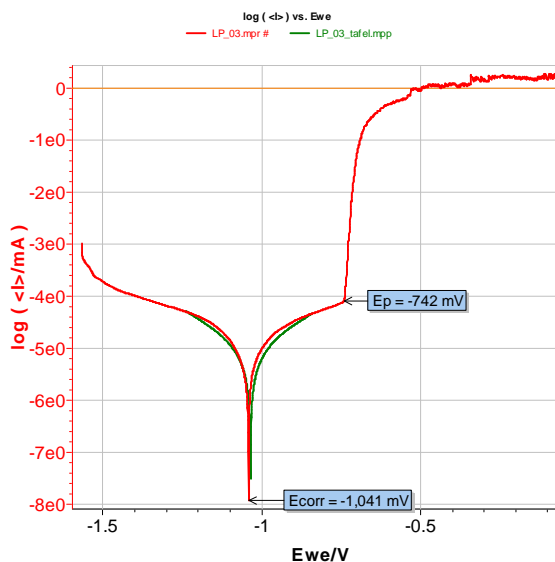


Fig. 5: LP curves of the electrode number 3 and its corresponding “Tafel Fit” window.

Table 1: Data resulting from LP investigations (Potentials are given in mV vs. Ag/AgCl).

Electrode	1	3	4	12
E_{corr}/mV	-1,152	-1,035	-1,124	-1,000
I_{corr}/nA	0.12	0.12	0.15	0.13
β_c/mV	265	306	290	323
β_a/mV	362	311	384	328
Corrosion rate /mmpy	0.13×10^{-3}	0.12×10^{-3}	0.15×10^{-3}	0.13×10^{-3}
E_p/mV	-760	-742	-746	-740

III-2 MPP investigations and Statistics

Parameters of MPP investigations are similar to those of LP investigations (Fig. 6). According to the results of LP investigations, I_p , which is the limiting current, is set to 50 μA .

Fig. 6: "Parameters Settings" window for MPP measurements.

MPP curves (Fig. 7) display the current shift due to the pitting process.

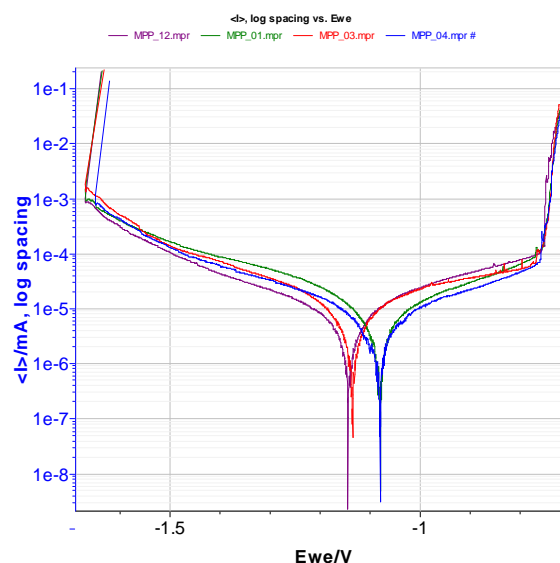


Fig. 7: MPP curves of the four electrodes.

E_p and E_{corr} are determined simultaneously via the "MultiPitting Statistics" function (Fig. 8). Note that E_{oc} of the "Multi Pitting Statistics" corresponds to E_{corr} . E_p and E_{corr} computed thank to this statistics tool, are in agreement with those obtained with Tafel Fit from LP results. Indeed, E_{corr} averages are -1,078 mV and -1,202 mV vs. Ag/AgCl for LP and MPP investigations respectively, and E_p averages are -747 mV and -716 mV vs. Ag/AgCl for LP and MPP investigations respectively.

channel	1	3	4	12
E init (V)	-1.417	-1.368	-1.353	-1.429
E oc (V)	-1.240	-1.163	-1.220	-1.183
Ep (V)	-0.716	-0.720	-0.714	-0.713

Fig. 8: "Multi Pitting Statistics" window in "Analysis" menu in EC-Lab® software.

IV- Conclusion

This note exhibits some corrosion techniques (LP and MPP) and corresponding analysis processes (“Tafel Fit” and “MultiPitting Statistics”). These tools are complementary. Indeed, “Tafel Fit” allows the user to obtain the corrosion rate and other typical corrosion parameters, whereas “MultiPitting Statistics” allows the user to compute data simultaneously from several data files.

Other investigations can be carried out with EC-Lab[®] software such as Critical Pitting Temperature with a thermostat controlled *via* EC-Lab[®] software.

References

- [1] Technical Notes #23, <http://www.bio-logic.info/potentiostat/notes.html>
- [2] Traité des Matériaux, Vol. 12 Corrosion et chimie de surfaces des métaux, D. Landolt, ed. Presses Polytechniques et Universitaire Romandes, 2003.
- [3] Cinétique électrochimique, J.-P. Diard, B. Le Gorrec, C. Montella, ed., Hermann (Paris) 1996.