

Fuel Cell Testing

Part I: Overview and I/E characterizations

I – INTRODUCTION

The fuel cell is defined as a device which produces electricity from fuel and oxidant. Fuel is provided at the anode and oxidant at the cathode. Unlike batteries, fuel cell can work continuously as long as it is provided with fuel and oxidant (no electrical charge is required after discharge). There are several types of fuel cell such as alkaline fuel cell, direct methanol fuel cell, phosphoric acid fuel cell, and proton exchange membrane fuel cell (PEMFC) [1,2]. PEMFC exhibits better performance at low temperature than the others, so lots of research are carried out on this kind of fuel cell. PEMFC is constituted as follows:

- anode (hydrogen oxidation, Fig. 1 eq 1),
- cathode (oxygen reduction, Fig. 1 eq 2),
- membrane allowing proton exchange between both sides.

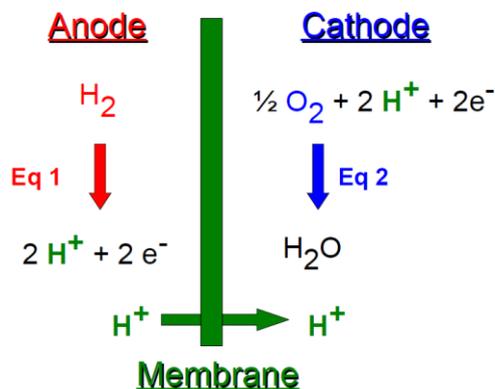


Figure 1: PEMFC principle.

Regarding fuel cell testing, a key issue is gas (specially gas temperature and humidity) and water management. These parameters are critical for reaching the optimal fuel cell performance.

The aim of this application note is to present the capabilities of the FCT series monitored by FC-Lab[®] software. This association allows user

to control gas, temperature, water and load box with high current ability (up to 150 A). Electrochemical Impedance Spectroscopy (EIS) will be discussed in another application note [3].

II – SET-UP DESCRIPTION

For this application note, FCT-150S with *automatic humidifier water filling and condenser purging* option was used. FCT-150S was monitored by FC-Lab[®] software. FCT-150S was connected to fuel cell according to the two-electrode connection (blue and white leads on the anode; red lead on the cathode).

The surface area of the fuel cell is 25 (if no indication) or 50 cm² (Fig. 2).



Figure 2: Fuel cell.

III – GAS AND WATER MANAGEMENT

III - 1 PRESENTATION

As previously stated, a key issue for fuel cell testing is the gas and water parameters such as gas flow, gas & water temperature, gas humidity, humidifier filling and condenser purge. These parameters are defined in the "Gas" tab (Fig. 3). In the block named "Cell", cell size, cell temperature and purge flow are set. The following three blocks deal with the supplied gas. Fuel cell can be feed by several gas combination such as H₂ and O₂, H₂ and Air or any other anodic gas (AG) and cathodic gas (CG). In the latter combination, user can adjust H₂ and O₂ *ratio*. Flow, humidifier


temperature, line temperature of anodic or cathodic gas have to be set in its respective block.

Note that stoichiometric (“stoichio”) mode can be selected *via* a combo box. If “stoichio” mode is chosen, user can adjust the stoichiometric coefficient for each gas.

Note the box “Humidifier automatic filling” has to be checked to activate this feature (Fig. 3).

Gas and water management data are stored in the “*.log” format file.

Figure 3: “Gas” window.

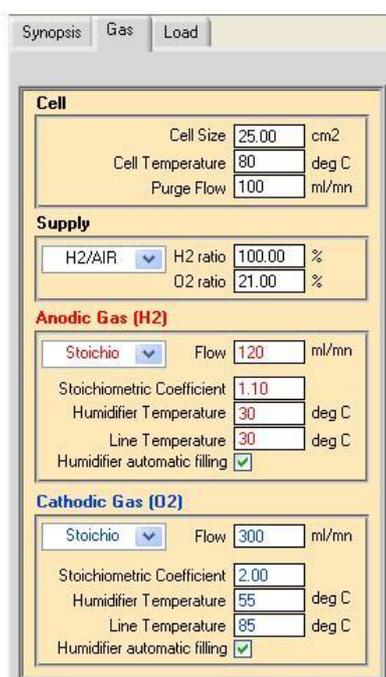

A global view of the gas and water management parameters is summarized in the “Synopsis” tab (Fig. 4).

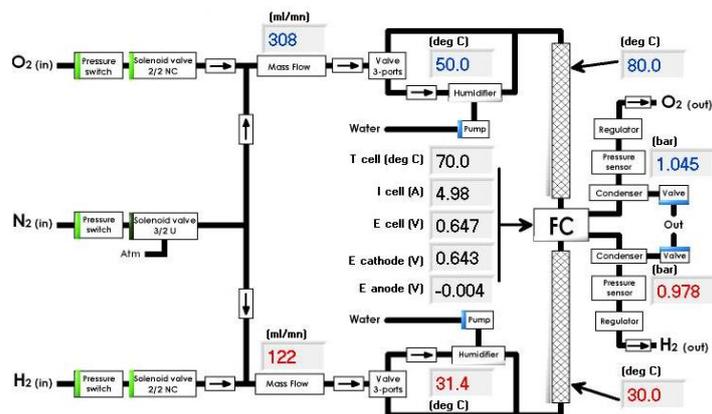


Figure 4: Synopsis tab.

III - 2 SAFETY PARAMETERS

To ensure safe investigations, temperature, pressure, flow, current or potential can be used as safety parameters in the “Security” window (Fig. 5).

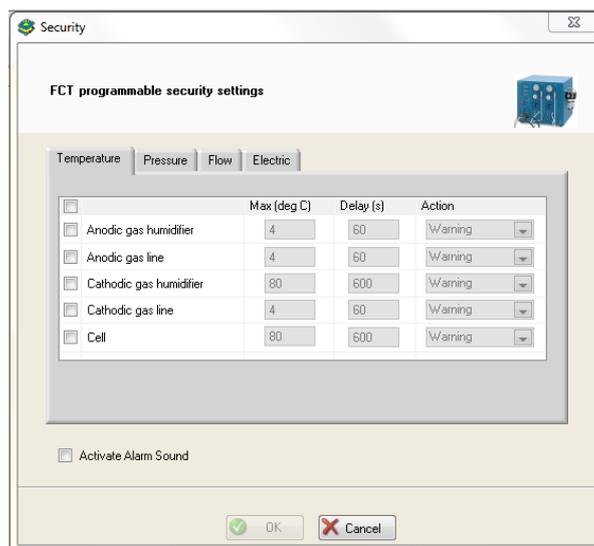


Figure 5: Security window (example is given with Temperature tab).

III - 3 HUMIDITY CALCULATOR TOOL

Humidity of gas affects strongly the fuel cell performance. That's why, in order to optimize fuel cell performance, FC-Lab® software enables the user to calculate the optimal humidity condition through the “Humidity Calculator” tool (Fig. 6) available in the “Help” menu of FC-Lab®.

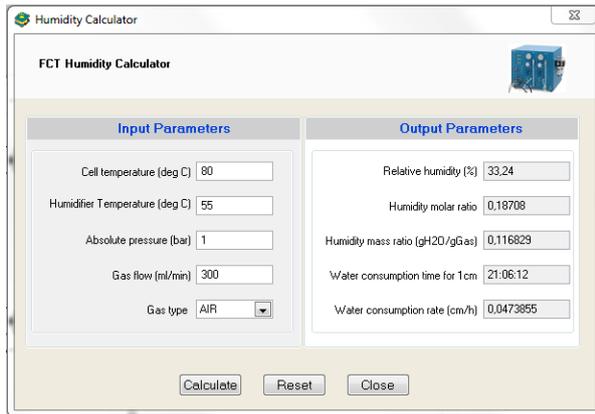


Figure 6: Humidity Calculator window.

IV – CHARACTERIZATIONS

To illustrate common fuel cell investigations, current polarization and pulses measurements are shown in this paragraph.

IV - 1 POLARIZATION

Polarization is performed at low current scan rate (few mA.cm⁻²) from current of zero to a limit value of potential, defined as $E_{we} < E_{min}$. Parameters are described in Fig. 7.

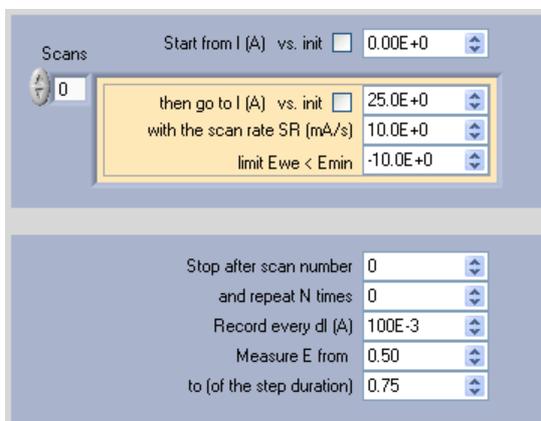


Figure 7: Polarization technique parameters window.

Resulting curves of E and P vs. current density (i) are displayed in Fig. 8.

Power is defined as follows:

$$P_i = E_i I_i \quad (1)$$

where P is the power, E the potential and I the current.

This E vs. I curve is usually divided in three regions [2]:

- Activation polarization: from 0 to 100 mA.cm⁻² (Fig. 8) in which reaction rate loss dominates,
- Ohmic polarization: from 100 to 600 mA.cm⁻² (Fig. 8) in which ohmic drop dominates,
- Concentration polarization: from 600 mA.cm⁻² to the end (Fig. 8) in which mass transfer dominates.

The fuel cell power vs. current can be plotted. In the example given in bottom of Fig. 8, the maximum power is 6.5 W and this maximum power is reached at 580 mA.cm⁻².

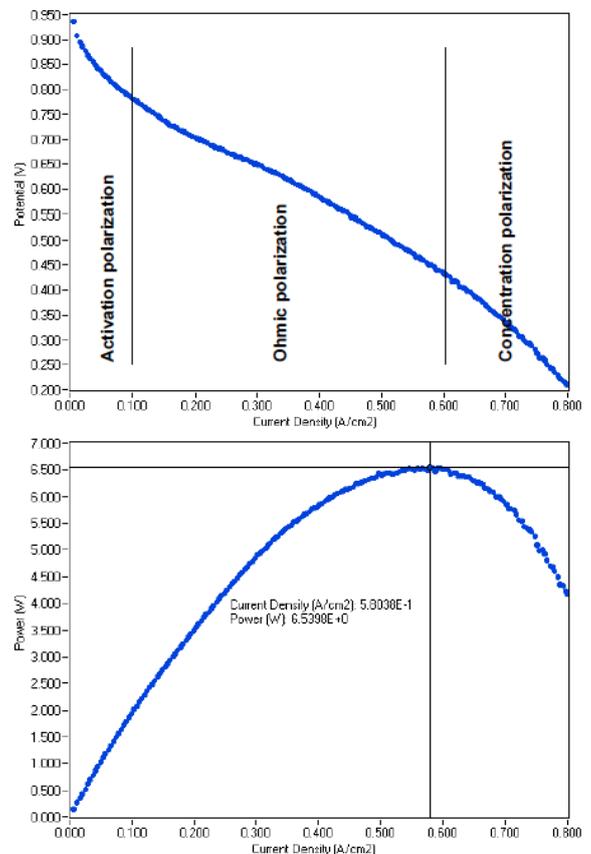


Figure 8: E (top) and P (bottom) vs. current density polarization curves.

IV - 2 CURRENT PULSE

In order to investigate fuel cell performance a discrete ramp of current can be applied. Two examples are given below. The first one illustrates the high current ability of the load box and the second one shows a long-term experiment.

a. High current

Successive current pulses of 60 s are applied to the fuel cell by step of 10 A (Fig. 9). In the first step, 10 A are applied, in the second 20 A and so on up to 100 A. Note that this experiment is carried out on a fuel cell with a surface area of 50 cm².

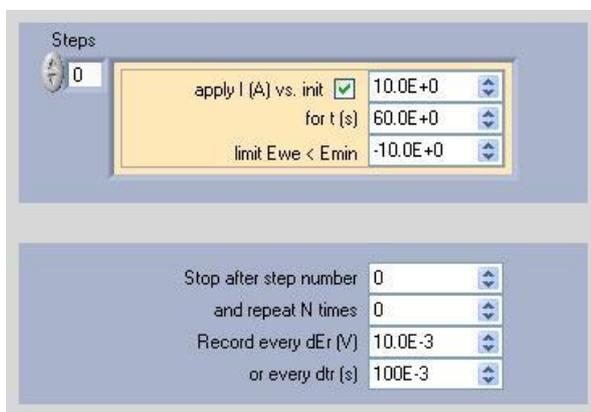


Figure 9: Current pulse technique parameters window.

Resulting chronopotentiometric curve is displayed in Fig. 10.

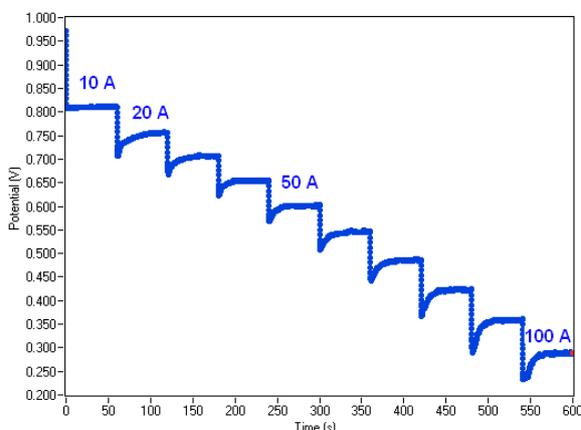


Figure 10: Chronopotentiometric curve.

b. Long term

Automatic gas and water managements allow user to perform long term measurements (thousands of hours). Current pulse technique with current intensity of 4, 5 and 2 A was performed over 60 h. The resulting chronopotentiometric curve (Fig. 11) shows the stability of the fuel cell potential during the experiment.

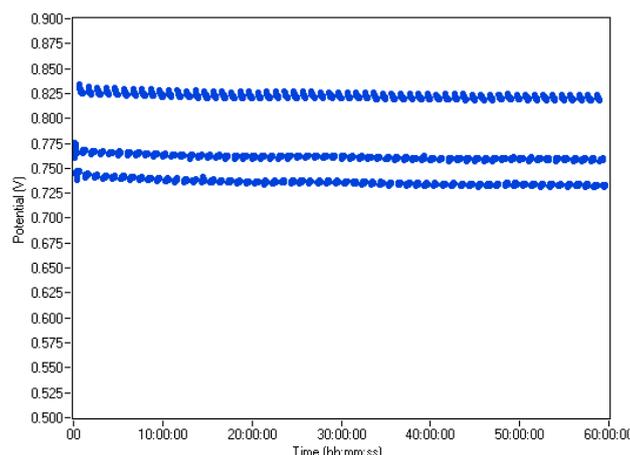


Figure 11: Long term chronopotentiometric curve.

VI – CONCLUSION

This note presents the advantage of the association of the FCT series compactness with the FC-Lab[®] monitoring software. This association makes possible to control the fluidic parts (gas and water) and electrochemical part (control and measure of current and potential) of the fuel cell testing with the same system.

Data files can be found in :

C:\Users\xxx\Documents\EC-Lab\Data\Samples\Battery\AN31-32_Manip

REFERENCES

- 1) J. Larminie, A. Dicks, *Fuel Cell Systems Explained*, Wiley, Chichester (2003).
- 2) H. R. Kunz, J. M. Fenton, *The Electrochem. Soc. Interface*, Fall (2004) 17.
- 3) [Application Note #32](#) "Fuel Cell Testing, Part II: EIS characterization"

Revised in 07/2018